This Page Is Inserted by IFW Operations and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.


Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS


IMAGES ARE BEST AVAILABLE COPY.


As rescanning documents will not correct images, please do not report the images to the Image Problem Mailbox.

791-

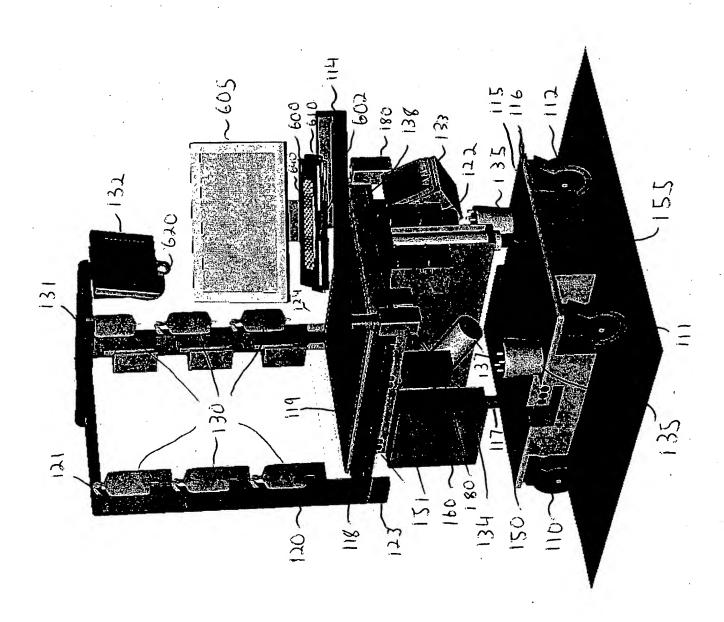



25

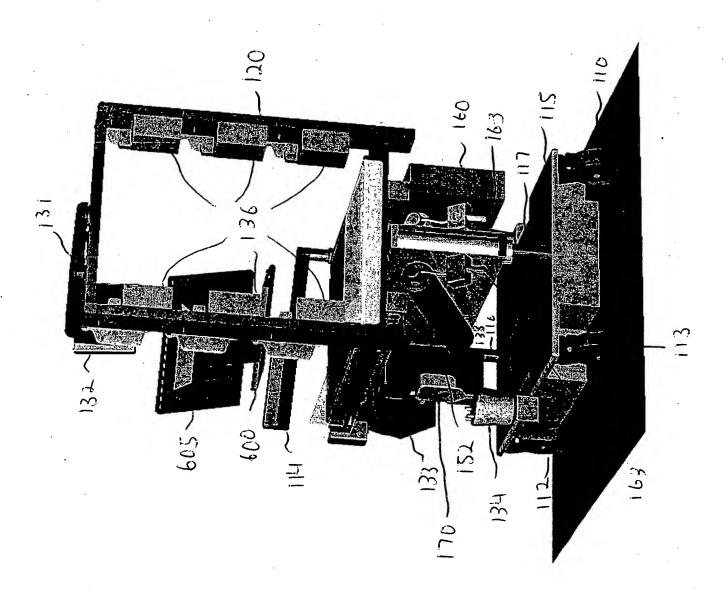

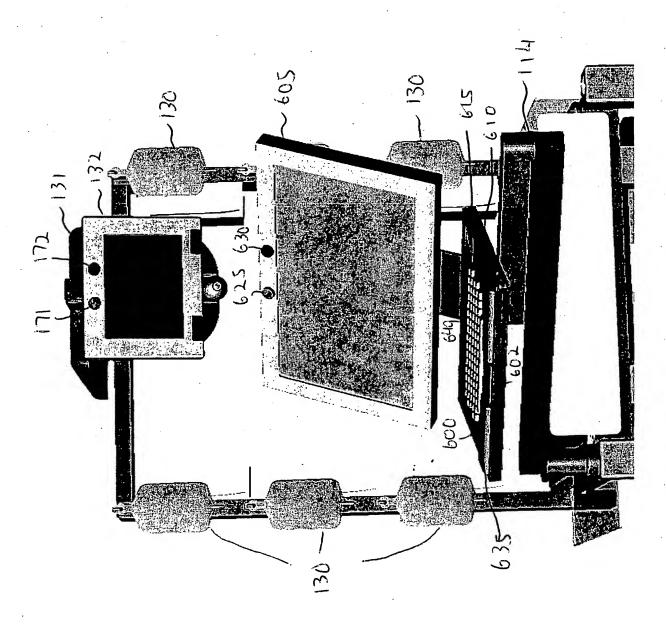

Title: Integrated Point-of-Care Systems and Methods Inventor: Baird M. Smith AttyDkt: PA2627US

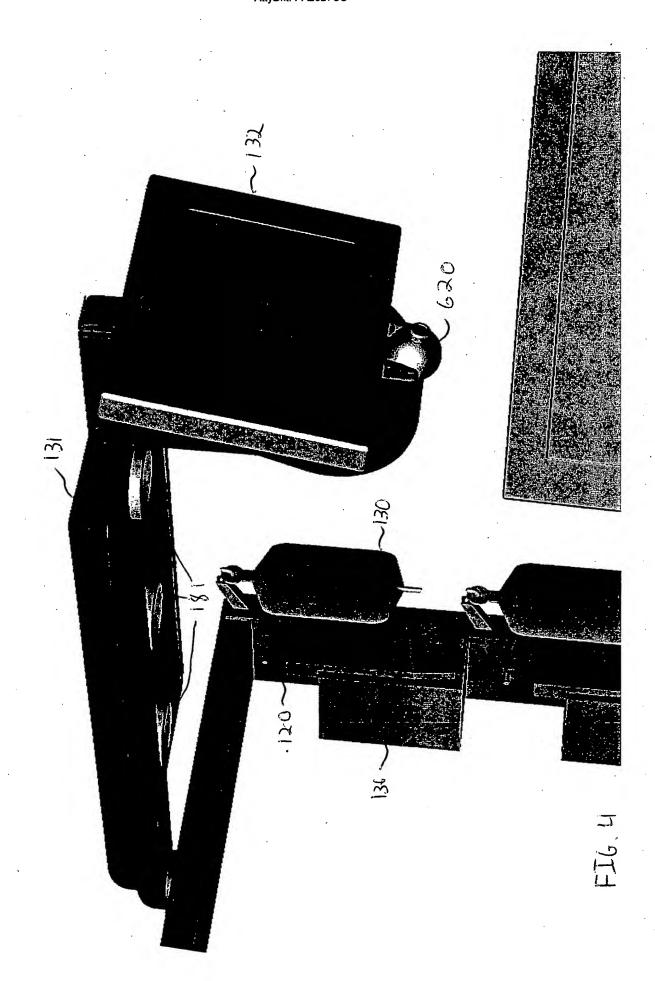

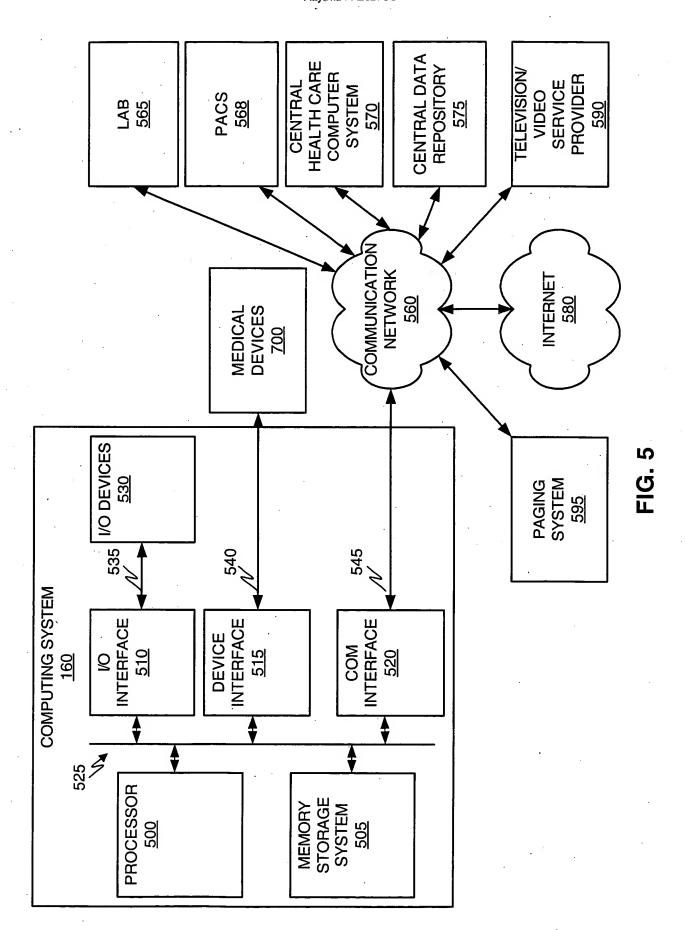

	DISPLAY DEVICE <u>605</u>	CAMERA <u>620</u>	READ-WRITE DATA DEVICE <u>635</u>	COLOR LIGHT SYSTEM 650
I/O DEVICES 530	COMPUTER MOUSE <u>602</u>	ID DEVICE 615	SPEAKER <u>630</u>	RADIO FREQUENCY CHIP IDENTIFIER 645
	KEYBOARD 600	BARCODE READER <u>610</u>	MICROPHONE 625	MAGNETIC CARD READER DEVICE <u>640</u>

MEDICAL DEVICES 700	MEDICAL MONITORING DEVICES 730	GLUCOSE MONITOR 736	NON-INV BLOOD PRESSURE MONITOR 742	CVP MONITOR 748	FLUID/AIR OUTPUT MONITORS 134-135	ARTMENT
		CARBON DIOXIDE MONITOR 734	INVASIVE BLOOD PRESSURE MONITOR 740	WEIGHT MONITOR 746	PULSE MONITOR 752	TISSUE COMPARTMENT PRESSURE MONITOR 758
		OXYGEN MONITOR 732	TEMP MONITOR 738	HEART MONITOR (EKG) 744	RESPIRATIO N MONITOR 750	CSF PRESSURE MONITOR 756
MEDICAL CARE DEVICES 710 VENTILATOR 136 136 INTRAVENOUS PUMP 131 DEFIBRILLATOR 718 FOOD PUMP 720						

Title: Integrated Point-of-Care Systems and Methods Inventor: Baird M. Smith

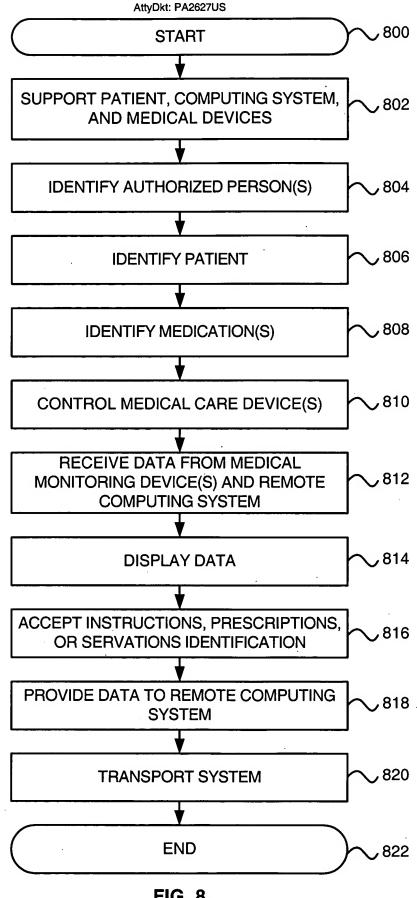


FIG. 8

Title: Integrated Point-of-Care Systems and Methods Inventor: Baird M. Smith AttyDkt: PA2627US

900

	MiBed22*	EI E
V(fal Signs) Name John Doe Resp 100/60 Resp 10 lippin O2 90 M/ appsain O2 90 M/ appsain Ferm Bary C Lippin Ferm Bary C Lippin Ferm Bary C Lippin All Projest	Ventilator Pressure - Volume Cycle 18- 19- 19- 19- 19- 19- 19- 19- 19- 19- 19	Pumps 1
PIVAII PROJECT CONTRACTOR CONTRACTOR		when 110:2016 PH When 110:20:16 PH

FIG. 9